

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 670 100 USP

Vol. flask, 1000 ml, NS 24, amber gl., USP, A, conf. cert.


Batch: 37-25

Serial:

Measuring Nr. 74784

Batch size: 86

Volume:	1000,0000 ml
Tolerance:	± 0,3000 ml
Average value:	999,7660 ml
Deviation:	0,0200 ml
Precision (CV):	0,0020 %

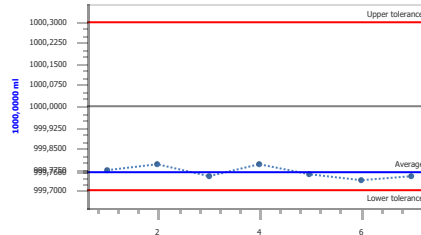

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	29.09.2025
Balance:	Sartorius - MSE14202S- OCE-D0

DE-M