

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 670 200

**Vol. flask, 2000 ml, NS 29, amber glass, A, conf. cert.**


**Batch:** 49-19

**Serial:**

**Measuring Nr.** 35239

**Batch size:** 88

|                        |                 |
|------------------------|-----------------|
| <b>Volume:</b>         | 2000,0000 ml    |
| <b>Tolerance:</b>      | $\pm 0,6000$ ml |
| <b>Average value:</b>  | 2000,2567 ml    |
| <b>Deviation:</b>      | 0,1062 ml       |
| <b>Precision (CV):</b> | 0,0053 %        |

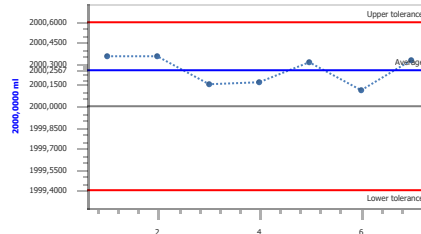

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|                  |                          |
|------------------|--------------------------|
| <b>Operator:</b> | 4                        |
| <b>Date:</b>     | 14.12.2019               |
| <b>Balance:</b>  | Sartorius - LC<br>6200 S |

DE-M