

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 051 BL

Grad. pipettes, 0,5:0,01 ml, blue grad., AS, conf. cert.




Batch: 49-20

Serial:

Measuring Nr. 43096

Batch size: 124

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
Tolerance:	± 0,0060 ml	± 0,0060 ml	± 0,0060 ml
Average value:	0,4971 ml	0,2997 ml	0,0993 ml
Deviation:	0,0009 ml	0,0010 ml	0,0011 ml
Precision (CV):	0,1789 %	0,3485 %	1,1074 %

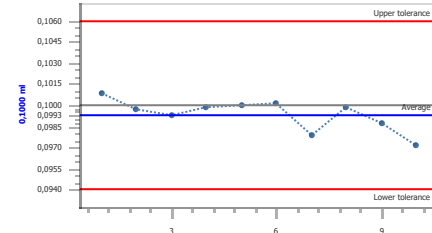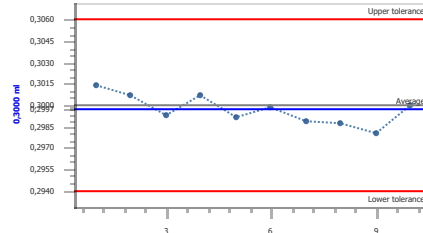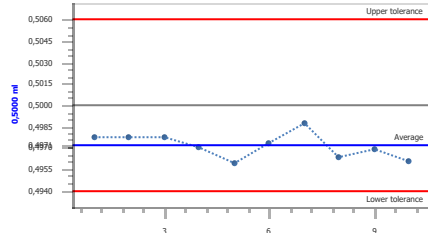

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	09.12.2020
Balance:	Sartorius - LE244S-OCE

