

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 051

Graduated pipettes, 0,5:0,01 ml, AS, conf. cert.




Batch: 50-23

Serial:

Measuring Nr. 65483

Batch size: 500

Volume:	0,5000 ml	0,3000 ml	0,1000 ml
Tolerance:	± 0,0060 ml	± 0,0060 ml	± 0,0060 ml
Average value:	0,5005 ml	0,3021 ml	0,1005 ml
Deviation:	0,0021 ml	0,0016 ml	0,0006 ml
Precision (CV):	0,4253 %	0,5289 %	0,5989 %

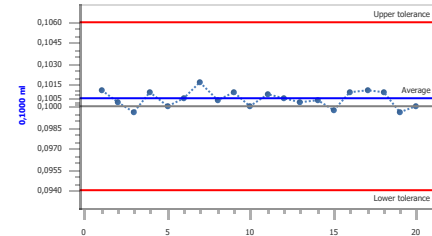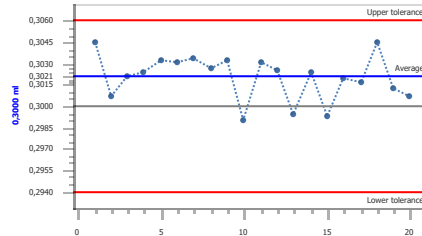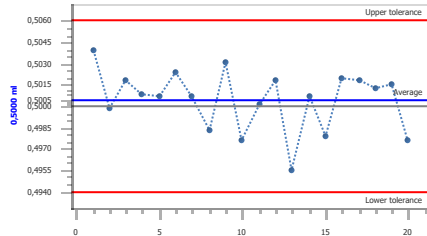

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	14.12.2023
Balance:	Sartorius - LE244S-OCE

