

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 110

Grad. pipettes, 1:0,1 ml, AS, conf. cert.




Batch: 25-24

Serial:

Measuring Nr. 67815

Batch size: 273

Volume:	1,0000 ml	0,6000 ml	0,2000 ml
Tolerance:	± 0,0070 ml	± 0,0070 ml	± 0,0070 ml
Average value:	0,9966 ml	0,5988 ml	0,2002 ml
Deviation:	0,0013 ml	0,0022 ml	0,0008 ml
Precision (CV):	0,1260 %	0,3731 %	0,4097 %

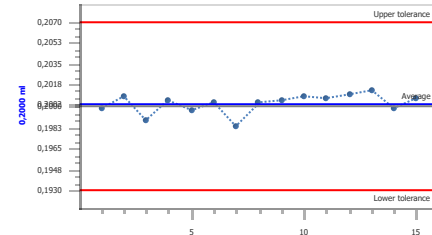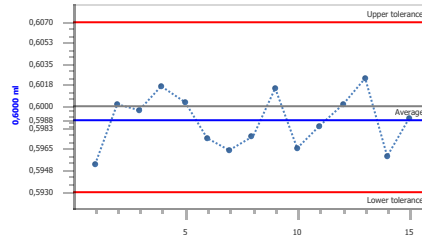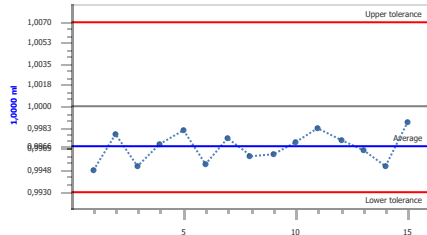

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	28.06.2024
Balance:	Sartorius - LE244S-OCE

