

# Certificate of performance



**Article:** 3 510 202

**Grad. pipettes, 2:0,02 ml, AS, conf. cert.**




**Batch:** 20-21

**Serial:**

**Measuring Nr.** 47245

**Batch size:** 3200

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	2,0007 ml	1,2006 ml	0,4011 ml
Deviation:	0,0025 ml	0,0023 ml	0,0016 ml
Precision (CV):	0,1244 %	0,1901 %	0,4032 %

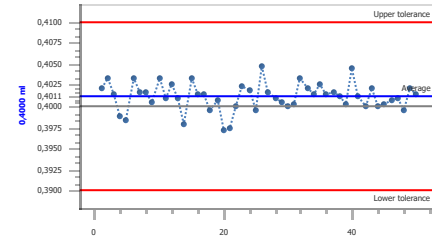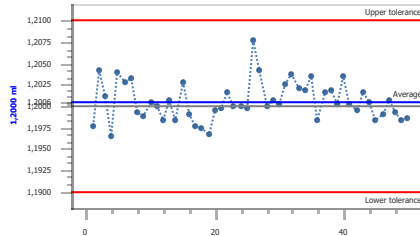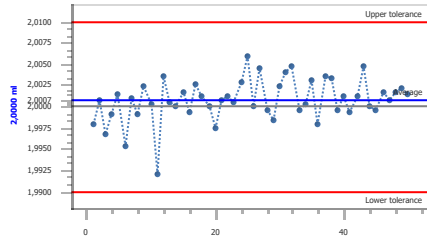

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	10.06.2021
Balance:	Sartorius - LE244S-OCE

