

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 202

**Grad. pipettes, 2:0,02 ml, AS, conf. cert.**




**Batch:** 09-22

**Serial:**

**Measuring Nr.** 53006

**Batch size:** 4165

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
<b>Tolerance:</b>	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
<b>Average value:</b>	1,9991 ml	1,1997 ml	0,4006 ml
<b>Deviation:</b>	0,0032 ml	0,0025 ml	0,0013 ml
<b>Precision (CV):</b>	0,1605 %	0,2120 %	0,3263 %

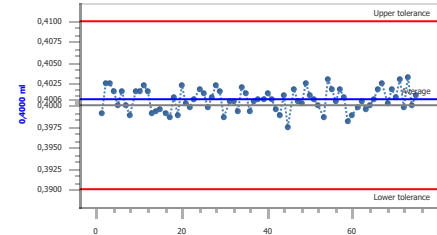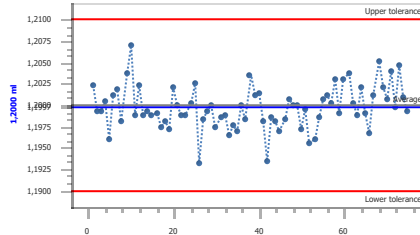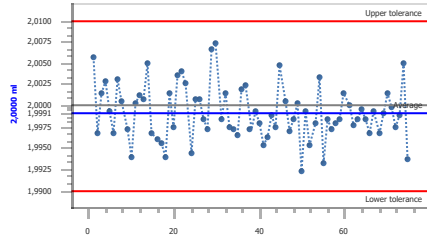

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	14.03.2022
<b>Balance:</b>	Sartorius - LE244S-OCE

