

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 505

Graduated pipettes, 5:0,5 ml, AS, conf. cert.




Batch: 35-17

Serial:

Measuring Nr.: 14092

Batch size: 2209

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	4,9933 ml	2,9970 ml	0,9994 ml
Deviation:	0,0048 ml	0,0069 ml	0,0034 ml
Precision (CV):	0,0965 %	0,2311 %	0,3364 %

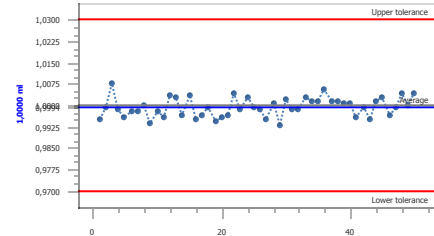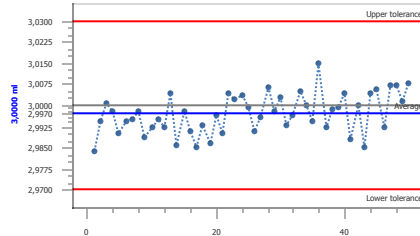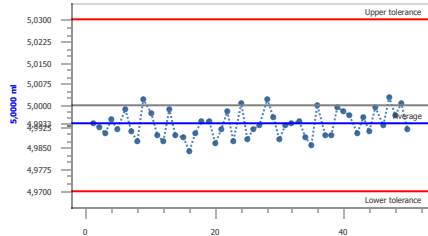

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	14.09.2017
Balance:	Sartorius - LE244S-OCE

