

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 505

Graduated pipettes, 5:0,05 ml, AS, conf. cert.




Batch: 15-18

Serial:

Measuring Nr. 20009

Batch size: 3200

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	$\pm 0,0300$ ml	$\pm 0,0300$ ml	$\pm 0,0300$ ml
Average value:	4,9977 ml	2,9981 ml	1,0001 ml
Deviation:	0,0068 ml	0,0057 ml	0,0028 ml
Precision (CV):	0,1363 %	0,1911 %	0,2786 %

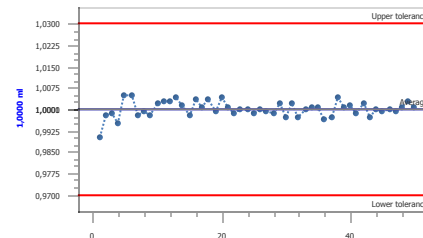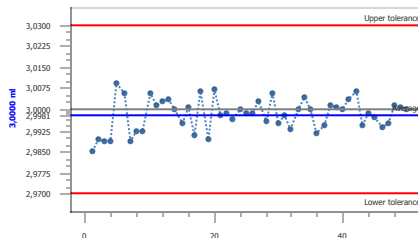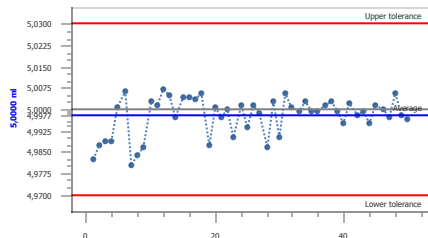

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

44

Date:

19.04.2018

Balance:

Sartorius -
LE244S-OCE

DE-M