

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 505

**Graduated pipettes, 5:0,05 ml, AS, conf. cert.**




**Batch:** 12-26

**Serial:**

**Measuring Nr.** 78214

**Batch size:** 2460

|                        |                  |                  |                  |
|------------------------|------------------|------------------|------------------|
| <b>Volume:</b>         | <b>5,0000 ml</b> | <b>3,0000 ml</b> | <b>1,0000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,0300$ ml  | $\pm 0,0300$ ml  | $\pm 0,0300$ ml  |
| <b>Average value:</b>  | 4,9906 ml        | 2,9956 ml        | 1,0020 ml        |
| <b>Deviation:</b>      | 0,0059 ml        | 0,0099 ml        | 0,0034 ml        |
| <b>Precision (CV):</b> | 0,1174 %         | 0,3300 %         | 0,3367 %         |

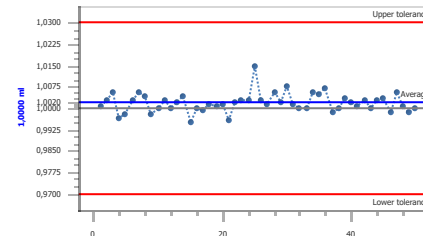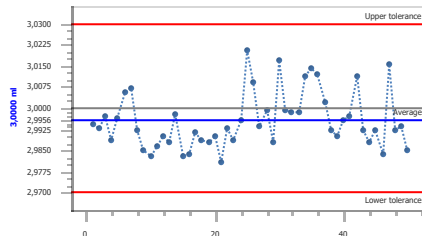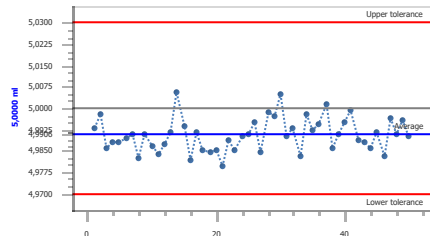

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

7

**Date:**

09.06.2026

**Balance:**

Sartorius -  
LE244S-OCE

DE-M