

# Certificate of performance



**Article:** 3 510 510

**Grad. pipettes, 5:0,1 ml, AS, conf. cert.**




**Batch:** 47-18

**Serial:**

**Measuring Nr.** 25901

**Batch size:** 1200

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
<b>Tolerance:</b>	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
<b>Average value:</b>	4,9917 ml	2,9952 ml	1,0007 ml
<b>Deviation:</b>	0,0062 ml	0,0053 ml	0,0024 ml
<b>Precision (CV):</b>	0,1249 %	0,1778 %	0,2418 %

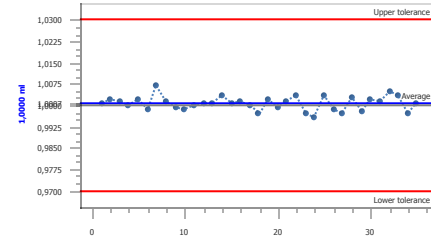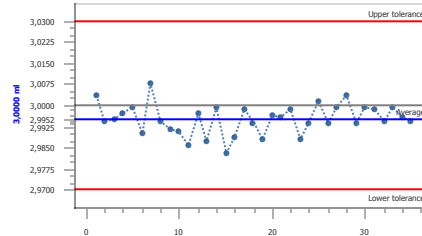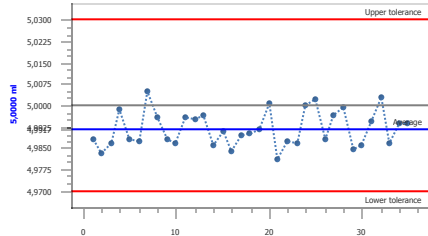

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	9
<b>Date:</b>	27.11.2018
<b>Balance:</b>	Sartorius - LE244S-OCE

