

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710

Graduated pipettes, 10:0,1 ml, AS, conf. cert.




Batch: 16-21

Serial:

Measuring Nr. 46422

Batch size: 5000

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	9,9949 ml	6,0043 ml	2,0035 ml
Deviation:	0,0073 ml	0,0068 ml	0,0053 ml
Precision (CV):	0,0733 %	0,1140 %	0,2654 %

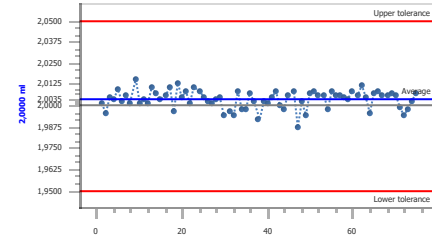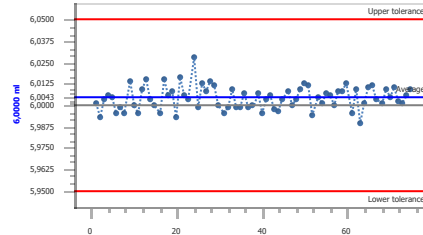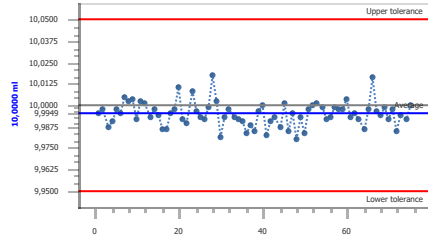

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	04.05.2021
Balance:	Sartorius - LE244S-OCE

