

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 710

Graduated pipettes, 10:0,1 ml, AS, conf. cert.




Batch: 45-21

Serial:

Measuring Nr. 50465

Batch size: 4513

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	9,9881 ml	5,9996 ml	2,0031 ml
Deviation:	0,0063 ml	0,0089 ml	0,0050 ml
Precision (CV):	0,0633 %	0,1477 %	0,2479 %

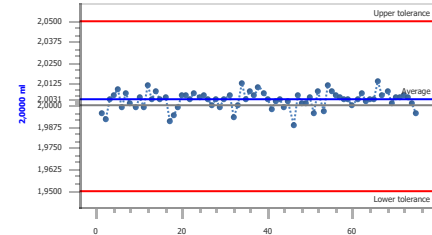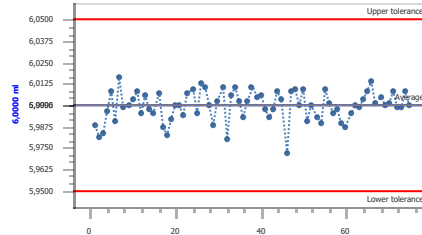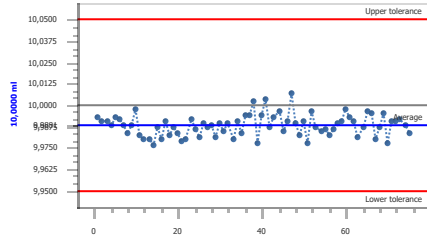

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	17.11.2021
Balance:	Sartorius - LE244S-OCE

