

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 810

Graduated pipettes, 20:0,1 ml, AS, conf. cert.




Batch: 44-19

Serial:

Measuring Nr. 34182

Batch size: 1142

Volume:	20,000 ml	12,000 ml	4,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	20,0024 ml	12,0021 ml	4,0060 ml
Deviation:	0,0145 ml	0,0169 ml	0,0096 ml
Precision (CV):	0,0724 %	0,1408 %	0,2408 %

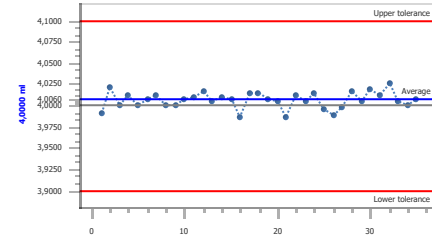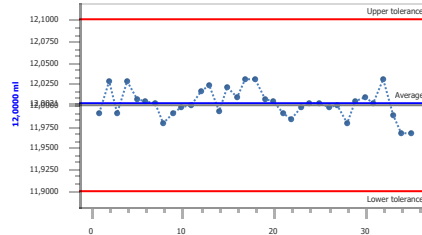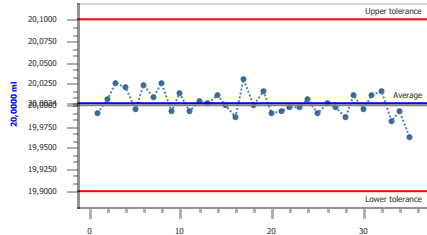

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	06.11.2019
Balance:	Sartorius - MSE224S-0CE -DU

