

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 510 810

**Graduated pipettes, 20:0,1 ml, AS, conf. cert.**




**Batch:** 05-24

**Serial:**

**Measuring Nr.** 66147

**Batch size:** 1200

Volume:	20,000 ml	12,000 ml	4,000 ml
<b>Tolerance:</b>	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
<b>Average value:</b>	19,9958 ml	11,9978 ml	4,0036 ml
<b>Deviation:</b>	0,0128 ml	0,0146 ml	0,0117 ml
<b>Precision (CV):</b>	0,0642 %	0,1217 %	0,2925 %

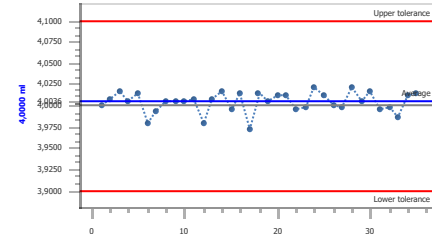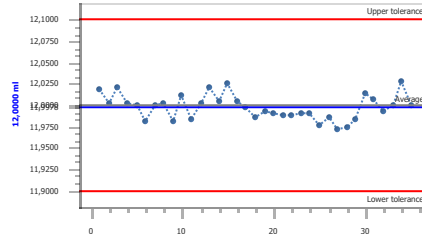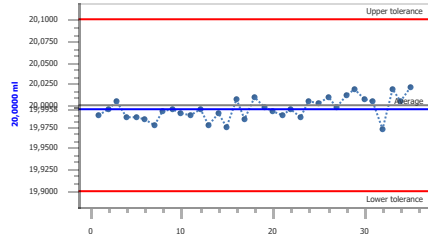

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	22.02.2024
<b>Balance:</b>	Sartorius - LE244S-OCE

