

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 510 910

Grad. pipettes, 25:0,1 ml, AS, conf. cert.




Batch: 07-26

Serial:

Measuring Nr. 76651

Batch size: 500

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	25,0351 ml	15,0400 ml	5,0228 ml
Deviation:	0,0193 ml	0,0131 ml	0,0078 ml
Precision (CV):	0,0771 %	0,0873 %	0,1552 %

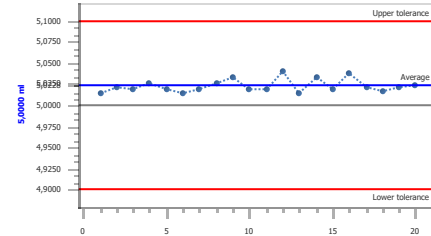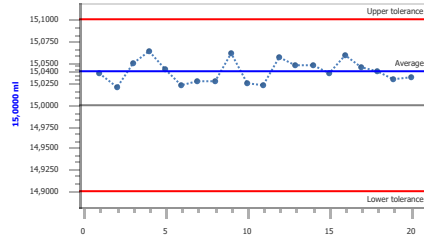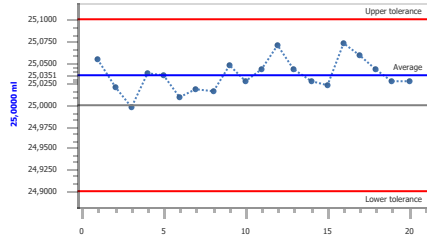

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	18.02.2026
Balance:	Sartorius - MSE224S-0CE -DU

