

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 515 710

**Grad. pipettes, 10:0,1 ml, AS, conf. cert.**




**Batch:** 25-23

**Serial:**

**Measuring Nr.** 63540

**Batch size:** 500

Volume:	10,000 ml	6,000 ml	2,000 ml
<b>Tolerance:</b>	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
<b>Average value:</b>	10,0043 ml	6,0054 ml	2,0054 ml
<b>Deviation:</b>	0,0120 ml	0,0067 ml	0,0054 ml
<b>Precision (CV):</b>	0,1196 %	0,1113 %	0,2678 %

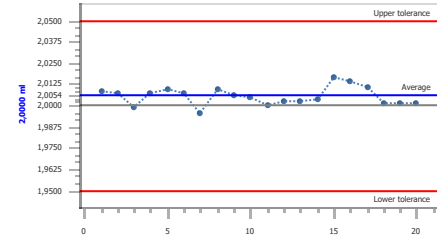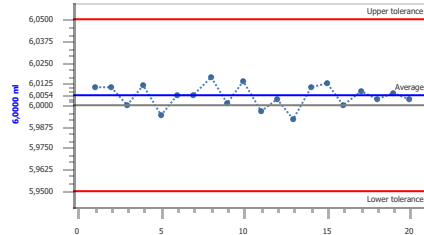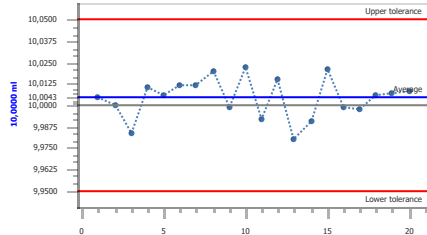

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 835

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

7

**Date:**

27.06.2023

**Balance:**

Sartorius -  
LE244S-OCE

DE-M