

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 005 USP

Volumetric pipettes, 0,5 ml, USP, AS, conf. cert.

Batch: 47-23


Serial:

Measuring Nr. 65424

Batch size:

131

Volume:	0,5000 ml
Tolerance:	$\pm 0,0060$ ml
Average value:	0,4992 ml
Deviation:	0,0007 ml
Precision (CV):	0,1337 %

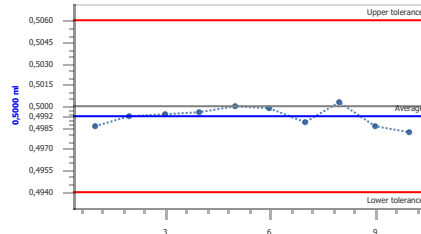

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

05.12.2023

Balance:

Sartorius -
LE244S-OCE

DE-M