

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 200 USP

Vol. pipette, 20 ml, USP, AS, conf. cert.


Batch: 22-19

Serial:

Measuring Nr. 30992

Batch size: 129

| | |
|------------------------|------------------|
| Volume: | 20,000 ml |
| Tolerance: | $\pm 0,0300$ ml |
| Average value: | 20,0039 ml |
| Deviation: | 0,0062 ml |
| Precision (CV): | 0,0311 % |

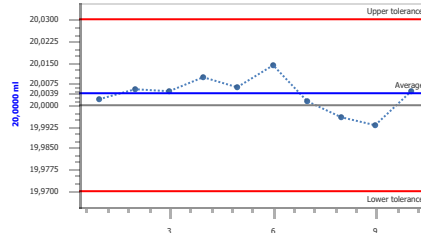

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator: 7

Date: 25.06.2019

Balance: Sartorius -
LE244S-OCE

DE-M