

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 555 005

Volumetric pipettes, 0,5 ml, 2 marks, AS, conf. cert.

Batch: 32-25


Serial:

Measuring Nr. 74709

Batch size:

1000

Volume:	0,5000 ml
Tolerance:	$\pm 0,0050$ ml
Average value:	0,4990 ml
Deviation:	0,0011 ml
Precision (CV):	0,2120 %

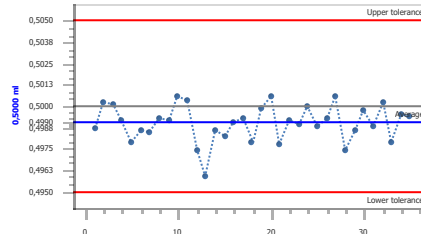

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

23.09.2025

Balance:

Sartorius -
LE244S-OCE

DE-M